





EMR Quick Reference Guide

Documentation – Arteriovenous Fistula


1. Go to '**Interactive View and Fluid Balance**' in the **Table of Contents (TOC)**

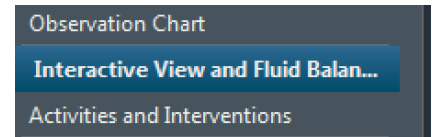


2. Select '**Adult Lines - Devices**' in the submenu

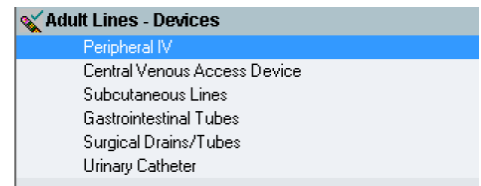


3. Click on the Customise View icon & select the '**Collapse All**' option at the bottom of folder.

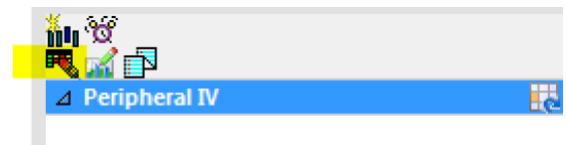


4. Tick boxes on the right side of '**Arteriovenous Access Device**' for 'On View' and 'Default Open' to allow options to be readily available and click on '**OK**'.

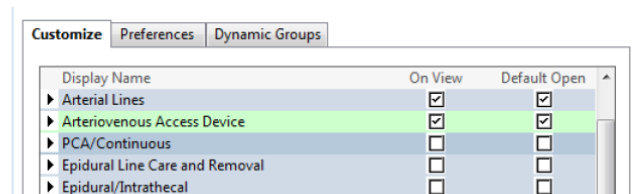

5. Click on the 'dynamic group' icon to enter the details of the **Arteriovenous Access Type**:

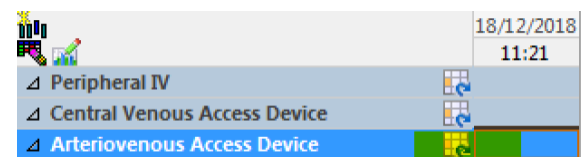

6. **Select AV Fistula**, arteriovenous access site, access laterality and click OK

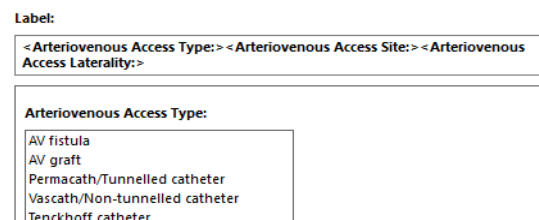

7. Documentation can now be completed in **iView**

