

# Devices – Documentation of Data in ICU through Devices




This Quick Reference Guide will explain how to:

Document in Interactive View through device association.


**Note: The Interactive View displays results in Actual time. To analyse data trends, the time interval display will need to be adjusted.**

## Recording Data from Device


1. Navigate to the relevant section in Interactive View i.e Vital Signs. Right click on the Date/Time header and select the frequency interval (e.g. 30 min or 1 hour).

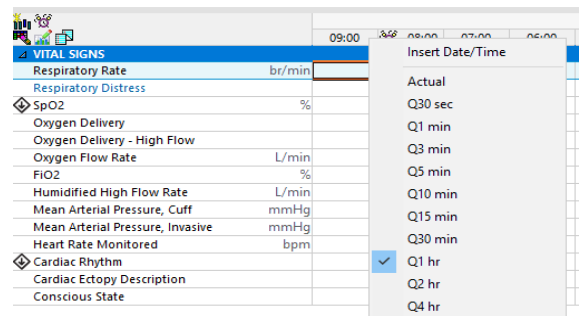

2. To obtain the data from the device, right click on the Date/Time header and select Insert Date/Time. If applicable, modify the date and time from Change Column Date/Time window. Click Ok.

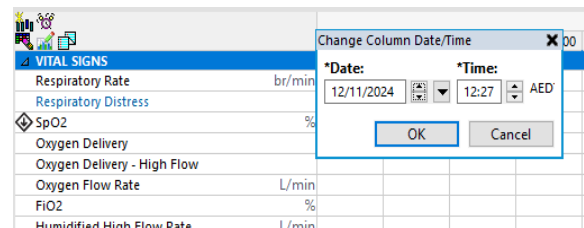

3. Double click the blue header under the selected time column. Values displayed on the monitor populate the patient chart in purple for verification. Review values, modify if required and manually enter any other data within the section.

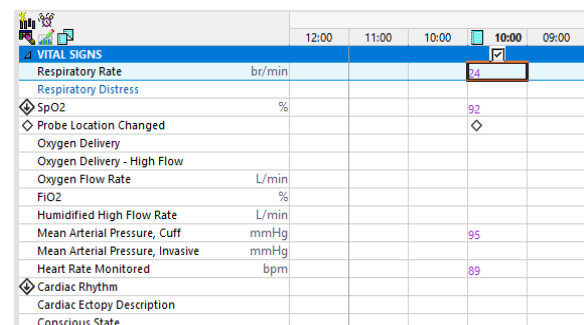

4. Click  green check icon to Sign. Verified data appears in black.



### Important

- This process must be followed for each of the individual observation bands relevant to the management of an ICU patient.
- Data may populate in multiple columns at certain times. If this occurs, consolidate the data into one column.